

UBAVET®

Animal health

DOSING AND ADMINISTRATION GUIDELINES



DAILY DOSAGE :	
WEIGHT	DOSAGE
DOGS	
0 - 5 KG (10 - 11 LB)	2 ML
5.1 - 10 KG (12 - 22 LB)	3 1/2 ML
10.1 - 15 KG (23 - 33 LB)	5 ML
15.1 - 20 KG (34 - 44 LB)	7 ML
20.1 - 30 KG (45 - 66 LB)	9 ML
30.1 - 50 KG (67 - 110 LB)	12 ML
50.1 KG+ (110.1 LB+)	15 ML
CATS	
	2 ML

ADJUST TO A MAINTENANCE DOSE AFTER 10-14 DAYS OF INITIAL DOES OR ACCORDING TO YOUR ANIMALS NEEDS.



DAILY DOSAGE :	
WEIGHT	DOSAGE
DOGS	
0 - 5 KG (10 - 11 LB)	2 ML
5.1 - 10 KG (12 - 22 LB)	3 1/2 ML
10.1 - 15 KG (23 - 33 LB)	5 ML
15.1 - 20 KG (34 - 44 LB)	7 ML
20.1 - 30 KG (45 - 66 LB)	9 ML
30.1 - 40 KG (67 - 88 LB)	11 ML
40.1 - 50 KG (89 - 110 LB)	14 ML
50.1 - 70 KG (110.1 - 154 LB)	18 ML
70.1 KG+ (154.1 LB+)	20 ML
CATS	
	2 ML

ADJUST TO A MAINTENANCE DOSE AFTER 10-14 DAYS OF INITIAL DOES OR ACCORDING TO YOUR ANIMALS NEEDS.

UBACAP + SYRINGE ADMINISTRATION USE AND MAINTENANCE


PLEASE FOLLOW THESE INSTRUCTIONS ON USING THE UBACAP™ PRESS-IN BOTTLE ADAPTOR AND SYRINGE.

HOW TO USE AND MAINTAIN UBAVET EXACT DOSE WITH SYRINGE ON UBAMEG, JOINT POWER MEG, JOINT PLUS AND UBAVIT SUPPLEMENTS.




OPEN BOTTLE

Open the bottle by turning the cap to the left (counter-clockwise) as shown. Remove and discard the seal off the top of the bottle (first time only).

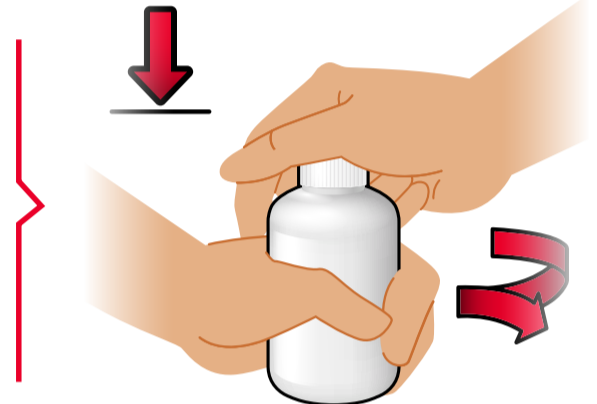

2

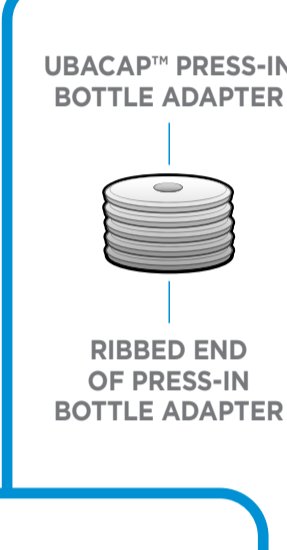

REMOVE SYRINGE AND UBACAP™ ADAPTER FROM PLASTIC OVERWRAP.

Keep syringe and adaptor. Discard clear plastic overwrap from bottle.

1

CLOSE LID AND SHAKE BOTTLE


Leaving the adaptor in place, return lid to bottle and turn to firmly close the lid. Vigorously shake the bottle for five seconds. Contents may separate, so shaking mixes them together again.



4

INSERT PRESS-IN BOTTLE ADAPTER

With the bottle on a flat surface, push the UBACAP™ press in bottle adaptor (with small hole upwards) all the way into the neck of the bottle with your thumbs while holding the bottle firmly.

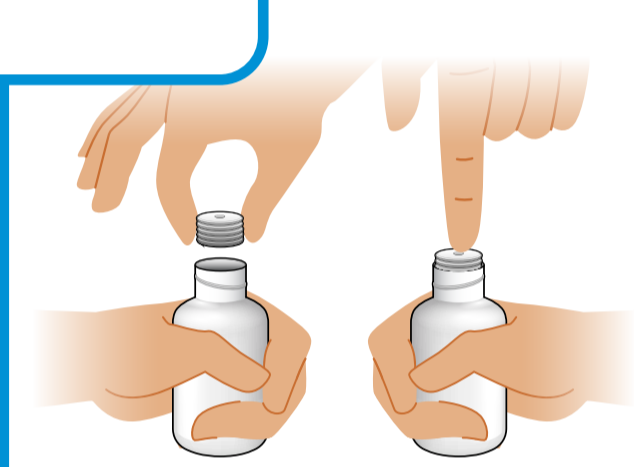


3

Note: Do not remove the press-in bottle adaptor from the bottle after it is inserted.

INSERT SYRINGE ONTO ADAPTOR


Remove lid from bottle. Insert the tip of the upright bottle through the opening of the press-in bottle adaptor until it is firmly in place.

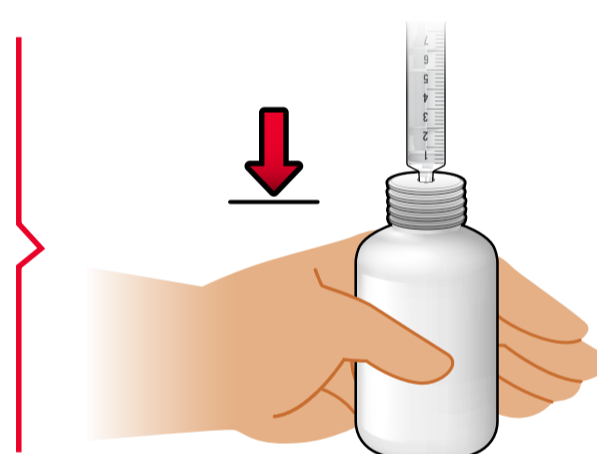

6

REMOVE AIR FROM SYRINGE


Push the syringe plunger all the way down to the tip of the syringe barrel to remove excess air.

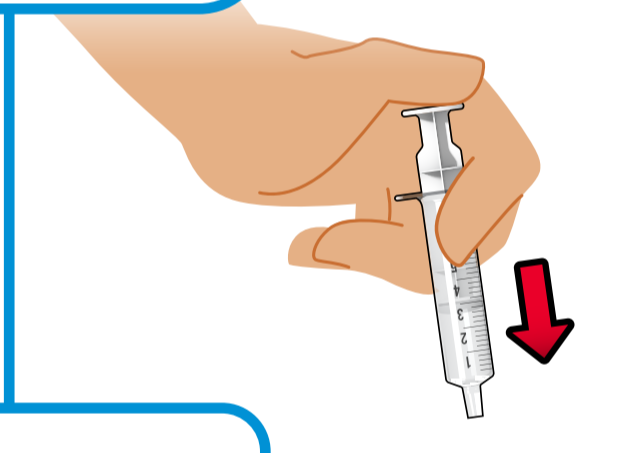

5

WITHDRAW DOSE FROM BOTTLE


With the syringe firmly in place, turn the bottle upside down. Pull down on the plunger until the bottom of the plunger is even with the markings on the syringe for your chosen dose (see bottle label for dosage). If you see large air spaces or bubbles, fully push the plunger in so that the oral solution flows back into the bottle, and repeat the above. Small bubbles are acceptable.

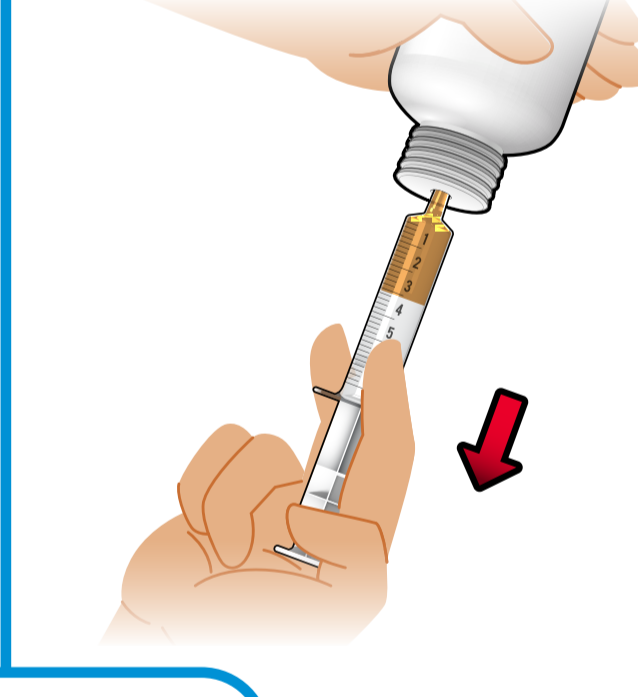

7

REMOVE SYRINGE


Turn the bottle upright. Remove the syringe from the press-in bottle adaptor and bottle by pulling straight up on the syringe barrel.

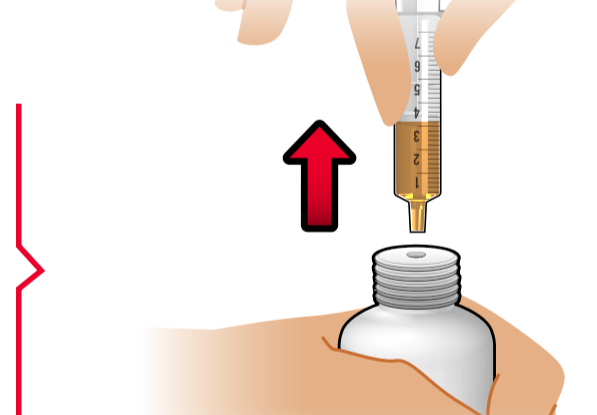

8

CHECK THE DOSE


Check that the correct dose was drawn up into the syringe. If the dose is not correct, insert the syringe tip firmly into the press-in bottle adaptor. Fully push in the plunger so that the liquid flows back into the bottle. Repeat Step 6 and Step 7.

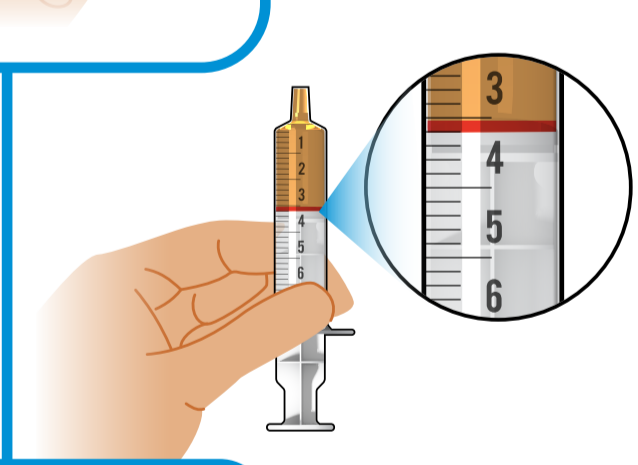

9

GIVE THE DOSE TO YOUR DOG OR CAT


Push the plunger to empty the syringe directly into the mouth or onto food.

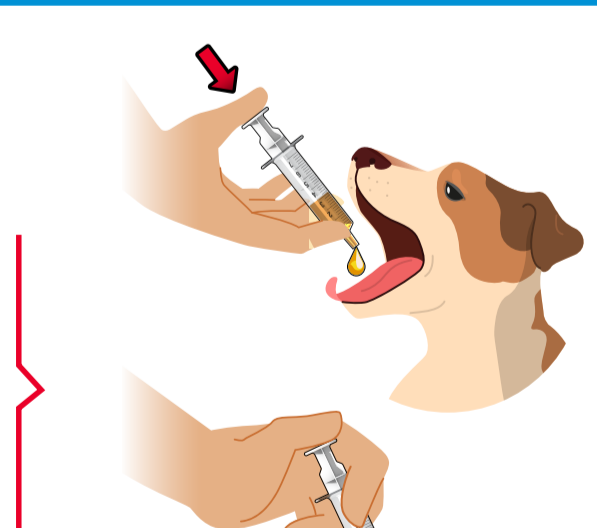

10

MAINTAINING AND CLEANING YOUR SYRINGE

If the syringe becomes blocked or seized, fill a cup with warm water and a little dish soap. Placing the nose of the syringe into the cup, proceed to push and pull the plunger, like a bicycle pump, to push the water through the syringe and to free up movement. Then repeat with warm water but without soap. Leave with plunger fully depressed and allow to air dry. Keep the syringe until bottle is empty, then discard.

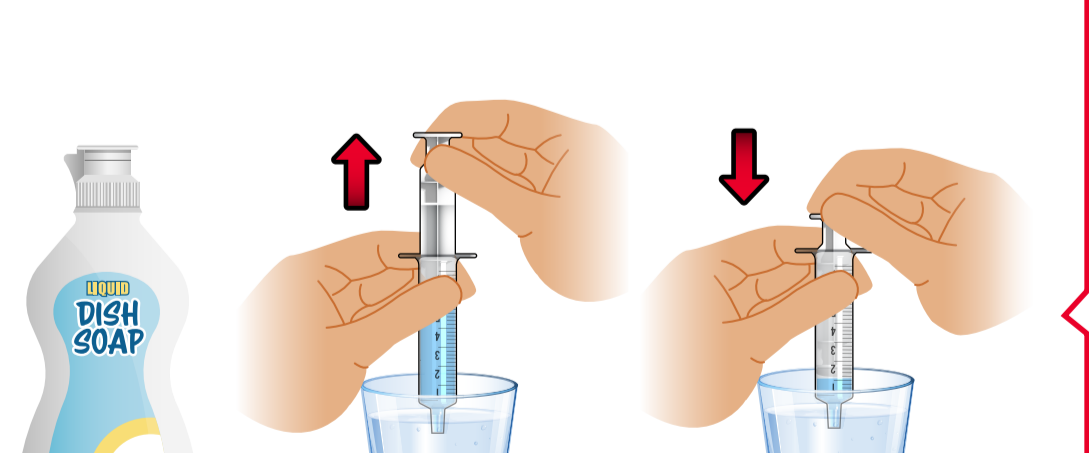

11

OPTIONAL TABLESPOON AND TEASPOON DOSING

If your syringe has stopped working please dose by tea and/or tablespoon. 1 measuring tablespoon has 15 mL, and one teaspoon has 5 mL of liquid.




*

Note: these are official, culinary measuring spoons. Dining spoons will vary.

STORAGE

Many UBAVET customers leave the syringe in the bottle instead using the screw on cap. Others prefer to use the screw on cap after each use. Both are acceptable.

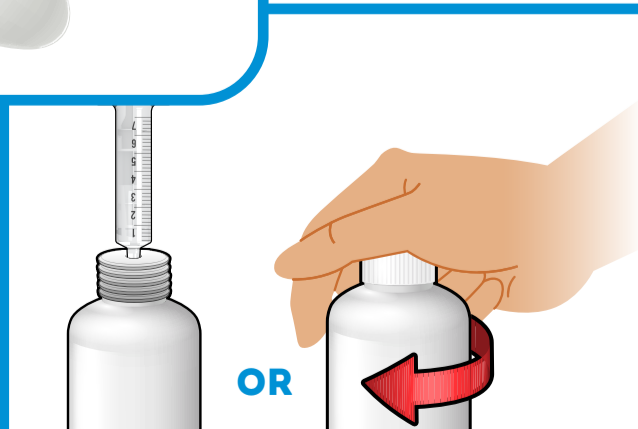

12

Store product at room temperature, away from direct sunlight. Shake well before each use.

FOR ADDITIONAL INFORMATION OR ASSISTANCE PLEASE CONTACT US:

INFO@UBAVET.COM

TOLL-FREE: 1-800-838-8563